



Development and evaluation of rapid novel isothermal amplification assays for important veterinary pathogens: *Chlamydia psittaci* and *Chlamydia pecorum*

Martina Jelocnik¹, Md. Mominul Islam¹, Danielle Madden¹, Cheryl Jenkins², James Branley³, Scott Carver⁴ and Adam Polkinghorne¹

¹ Centre for Animal Health Innovation, University of the Sunshine Coast, Maroochydore, Queensland, Australia

² NSW Department of Primary Industries, Elizabeth Macarthur Agricultural Institute, Menangle, New South Wales, Australia

³ Nepean Hospital, Penrith, New South Wales, Australia

⁴ School of Biological Sciences, University of Tasmania, Hobart, Tasmania, Australia

ABSTRACT

Background. *Chlamydia psittaci* and *Chlamydia pecorum* are important veterinary pathogens, with the former also being responsible for zoonoses, and the latter adversely affecting koala populations in Australia and livestock globally. The rapid detection of these organisms is still challenging, particularly at the point-of-care (POC). In the present study, we developed and evaluated rapid, sensitive and robust *C. psittaci*-specific and *C. pecorum*-specific Loop Mediated Isothermal Amplification (LAMP) assays for detection of these pathogens.

Methods and Materials. The LAMP assays, performed in a Genie III real-time fluorometer, targeted a 263 bp region of the *C. psittaci*-specific *Cps_0607* gene or a 209 bp region of a *C. pecorum*-specific conserved gene *CpecG_0573*, and were evaluated using a range of samples previously screened using species-specific quantitative PCRs (qPCRs). Species-specificity for *C. psittaci* and *C. pecorum* LAMP targets was tested against DNA samples from related chlamydial species and a range of other bacteria. In order to evaluate pathogen detection in clinical samples, *C. psittaci* LAMP was evaluated using a total of 26 DNA extracts from clinical samples from equine and avian hosts, while for *C. pecorum* LAMP, we tested a total of 63 DNA extracts from clinical samples from koala, sheep and cattle hosts. A subset of 36 *C. pecorum* samples was also tested in a thermal cycler (instead of a real-time fluorometer) using newly developed LAMP and results were determined as an end point detection. We also evaluated rapid swab processing (without DNA extraction) to assess the robustness of these assays.

Results. Both LAMP assays were demonstrated to species-specific, highly reproducible and to be able to detect as little as 10 genome copy number/reaction, with a mean amplification time of 14 and 24 min for *C. psittaci* and *C. pecorum*, respectively. When testing clinical samples, the overall congruence between the newly developed LAMP assays and qPCR was 92.3% for *C. psittaci* (91.7% sensitivity and 92.9% specificity); and 84.1% for *C. pecorum* (90.6% sensitivity and 77.4% specificity). For a subset of 36 *C. pecorum* samples tested in a thermal cycler using newly developed LAMP, we

Submitted 20 July 2017
Accepted 22 August 2017
Published 8 September 2017

Corresponding author
Martina Jelocnik,
Martina.jelocnik@research.usc.edu.au

Academic editor
Joseph Gillespie

Additional Information and
Declarations can be found on
page 16

DOI 10.7717/peerj.3799

© Copyright
2017 Jelocnik et al.

Distributed under
Creative Commons CC-BY 4.0

OPEN ACCESS

observed 34/36 (94.4%) samples result being congruent between LAMP performed in fluorometer and in thermal cycler. Rapid swab processing method evaluated in this study also allows for chlamydial DNA detection using LAMP.

Discussion. In this study, we describe the development of novel, rapid and robust *C. psittaci*-specific and *C. pecorum*-specific LAMP assays that are able to detect these bacteria in clinical samples in either the laboratory or POC settings. With further development and a focus on the preparation of these assays at the POC, it is anticipated that both tests may fill an important niche in the repertoire of ancillary diagnostic tools available to clinicians.

Subjects Microbiology, Veterinary Medicine, Public Health

Keywords *Chlamydia psittaci*, *Chlamydia pecorum*, LAMP, Diagnostics, Rapid tests, Clinical samples

INTRODUCTION

The obligatory intracellular bacteria, *Chlamydia psittaci* and *Chlamydia pecorum*, are globally widespread veterinary pathogens that cause disease in an astonishing range of hosts. *C. psittaci*, the causative agent of psittacosis or wasting bird disease, is regarded as a major economically relevant poultry and pet bird pathogen (Knittler & Sachse, 2015; Szymanska-Czerwinska & Niemczuk, 2016). Globally, *C. psittaci* infections are also sporadically reported in other animal species such as pigs, cattle, sheep and horses, resulting in asymptomatic shedding, acute respiratory disease and, in the case of horses, reproductive loss (Reinhold, Sachse & Kaltenboeck, 2011; Knittler & Sachse, 2015; Jelocnik et al., 2017). Importantly, this pathogen continues to pose risks to public health through zoonotic transmission events that may lead to severe pneumonia (Gaede et al., 2008; Laroucau et al., 2015; Branley et al., 2016). This zoonotic risk is typically associated with direct contact with *C. psittaci* infected birds, although indirect contact through exposure to environmental contamination has been suggested (Branley et al., 2014; Branley et al., 2016).

C. pecorum is perhaps best known as the major pathogen of the iconic Australian native species, the koala. These infections are most commonly asymptomatic but can also result in serious inflammatory ocular and/or urogenital disease, affecting almost all Australia's mainland koala populations (Polkinghorne, Hanger & Timms, 2013; Gonzalez-Astudillo et al., 2017). *C. pecorum* is also an important livestock pathogen causing a range of debilitating diseases such as sporadic bovine encephalomyelitis, polyarthritis, pneumonia and conjunctivitis, with faecal shedding as a constant feature of these infections (Lenzko et al., 2011; Reinhold, Sachse & Kaltenboeck, 2011; Walker et al., 2015). In livestock, chlamydial pathogens such as *C. pecorum* and *C. psittaci* may be found as co-infections, raising the possibility of a synergistic pathogenic effect (Lenzko et al., 2011; Reinhold, Sachse & Kaltenboeck, 2011; Knittler & Sachse, 2015). The reports of chlamydial infections in novel hosts and their recognised pathogenic potential (Jelocnik et al., 2015b; Burnard & Polkinghorne, 2016; Taylor-Brown & Polkinghorne, 2017), further highlight the need for faster detection and molecular discrimination of infecting strains.

Whilst significant progress has been made in understanding the molecular epidemiology of *C. psittaci* and *C. pecorum* infections (Jelocnik et al., 2015a; Branley et al., 2016), the diagnosis and detection of these pathogens is still difficult, laborious and costly, challenging efforts to manage and treat infected hosts. A variety of traditional (cell culture, antigen detection, and serology) and molecular (conventional and real-time quantitative PCR (qPCR)) diagnostic options are used to detect chlamydial infections and diagnose chlamydiosis (Sachse et al., 2009). For both *C. psittaci* and *C. pecorum*, nucleic acid amplification tests (NAATs) are presently considered the diagnostic “gold standard” due to their specificity and sensitivity, however the use of these assays is mainly restricted to research and/or diagnostic laboratories. In the absence of standardised gene target(s) for these organisms, numerous single or nested species-specific qPCR assays have been proposed and/or are used for *C. psittaci* (Madico et al., 2000; Geens et al., 2005; Menard et al., 2006; Branley et al., 2008) and *C. pecorum* (Marsh et al., 2011; Higgins et al., 2012; Wan et al., 2011; Walker et al., 2016) diagnosis.

The development and use of low-cost molecular diagnostic tools performed at the point-of-care (POC) which fulfil the World Health Organization “ASSURED” criteria of affordable, sensitive, specific, user-friendly, rapid, equipment-free, and deliverable to those in need to be tested, are on the exponential rise (Maffert et al., 2017). While POC testing is not necessarily required when considering most chlamydial infections of veterinary concern, the ability to provide a rapid detection of infections becomes of increasing significance when veterinarians and other animal workers may be at risk of being exposed to *C. psittaci* infections in field or farm settings. POC testing is also particularly relevant for *Chlamydia* screening in wild animals where laboratory testing is not accessible either due to logistics associated with field sampling or that services are not routinely available for testing of samples from wildlife. The latter problem is particularly acute for diagnosing infections in koalas, with the recent decision to stop the production of a commercially viable solid-phase ELISA leaving wildlife hospitals unable to diagnose and successfully treat asymptomatic *C. pecorum* infections (Hanger et al., 2013).

While there are many options for molecular POC diagnostics, Loop Mediated Isothermal Amplification (LAMP) assays developed for use in pathogen diagnostics are popular as they offer significant advantages over PCR and/or serology testing (Maffert et al., 2017). Rapid, simple, highly specific, easy to interpret, and carried out at a constant temperature, LAMP assays can provide a diagnosis in 30 min, in either laboratory or field setting (Mansour et al., 2015; Notomi et al., 2015). Rapid isothermal LAMP assays that could be performed at the POC targeting human *C. pneumoniae* (Kawai et al., 2009) and *C. trachomatis* (Jevtusevska et al., 2016; Choopara et al., 2017) infections have been proposed for use in chlamydial diagnostics. Development of a *C. pecorum* LAMP, in particular, would meet immediate demand for koala *C. pecorum* infections diagnostics, providing an alternative solution for the current laboratory diagnostics. A recent outbreak of psittacosis in veterinary staff and students in contact with a *C. psittaci*-infected and sick neonatal foal (Chan et al., 2017; Jelocnik et al., 2017), further demonstrates the need for POC assays such as LAMP to rapidly diagnose *C. psittaci*. In the present study, we describe the development and evaluation of

rapid and robust *C. psittaci*-specific and *C. pecorum*-specific LAMP assays for detection of these organisms in either laboratory or POC settings.

MATERIALS AND METHODS

Bacterial cultures and clinical samples used in this study

C. psittaci LAMP assay was evaluated using: (1) 12 DNA samples extracted from previously characterised *C. psittaci* isolates (10 human, two parrot and one equine) (Table S1); (2) DNA extracted from 21 placental, foetal, nasal, lung and rectal swabs, and 1 each placental and foetal tissue sample taken from 20 equine hosts; and (3) three pigeon liver DNA extracts (Table S2). All samples were collected and submitted as part of routine diagnostic testing by field or district veterinarians to the State Veterinary Diagnostic Laboratory (SVDL), Elizabeth Macarthur Agricultural Institute (EMAI), Menangle, NSW, Australia, and as such do not require special animal ethics approval. DNA extracts from these samples were kindly provided by Dr. Cheryl Jenkins, and Dr. James Branley. The use of these swabs was considered by the University of The Sunshine Coast (USC) Animal Ethics Committee and the need for further ethics consideration was waived under exemption AN/E/17/19.

C. pecorum LAMP was evaluated using a: (1) 18 DNA samples extracted from previously characterised koala ($n = 7$), sheep ($n = 4$), cattle ($n = 4$) and pig *C. pecorum* ($n = 3$) cultures (Table S1); (2) 16 sheep and 13 cattle ocular, rectal, and tissue swab DNA samples; and (3) 34 ocular and urogenital (UGT) koala swab DNA samples (Table S3), all available in our collection. The use of these swabs, also collected by qualified veterinarians as a part of routine diagnostic testing, was considered and approved for exemption by the University of The Sunshine Coast (USC) Animal Ethics Committee (AN/E/14/01 and AN/E/14/31).

We also evaluated the specificity of the assays against DNA samples extracted from previously characterised (i) chlamydial isolates (koala *C. pneumoniae* LPCoIN, *C. abortus* S26/3, *C. suis* S45, *C. trachomatis* serovar D, *C. murridarum* Nigg, *C. caviae* GPIC) and uncultured *Chlamydiales* (*Fritschea* spp.); (ii) Gram negative *Escherichia coli* and *Prevotella bivia*; Gram positive *Fusobacterium nucleatum*, *Staphylococcus epidermidis*, *S. aureus*, *Streptococcus* spp., and *Enterococcus faecalis*; and (iii) commercially available human gDNA (Promega, Alexandria, NSW 2015), all available in our laboratory (Table S1).

In order to evaluate rapid swab processing, 18 ocular, cloacal and UGT (14 dry and four RNA-Later) clinical swabs taken from 14 koalas with presumptive chlamydiosis were used for testing without DNA extraction. Briefly, RNA-Later and dry swabs with added 500 μ L TE buffer were vortexed vigorously for 5 min. 300 μ L aliquots were then heated to 98 °C for 15 min to lyse DNA, following LAMP testing. The use of these swabs, collected as a part of routine diagnostic testing, is also under Animal Ethics approval exemption (AN/E/14/01). An aliquot of 50 μ L of the swab suspension was used for LAMP and qPCR assays, while from the remaining volume of the swab suspension was used for DNA extraction, in order to compare swab suspension and its paired extracted DNA as a template in the assays.

LAMP assays design

For the *C. psittaci*-specific LAMP gene target, we targeted a previously described conserved single-copy *C. psittaci*-specific CDS, encoding for hypothetical protein and denoted

Cpsit_0607 in the representative *C. psittaci* 6BC strain (Genbank accession number [NC_015470.1](#)) ([Voigt, Schöfl & Saluz, 2012](#)). This gene was also previously proposed as a target for molecular diagnosis of *C. psittaci* infections ([Opota et al., 2015](#)).

The *C. pecorum*-specific candidate LAMP gene target, encoding for a single-copy conserved hypothetical protein and denoted *CpecG_0573* in the *C. pecorum* MC/Marsbar koala type strain (GenBank accession number [NZ_CM002310.1](#)), was selected based on a comparative genomics analysis of published koala and livestock *C. pecorum* genomes ([Jelocnik et al., 2015a](#)). For the purposes of this study, we will refer to it as *Cpec_HP*. Both candidate gene sequences were aligned to the corresponding allele from other publicly available *C. psittaci* or *C. pecorum* strains using Clustal X (as implemented in Geneious 9 ([Kearse et al., 2012](#))), and analysed in blastn against the nucleotide collection nr/nt database to assess intra-species sequence identity, and inter-species specificity.

For *C. ps_0607* alignment, besides 6BC, we used the gene alleles from strains 84/55 ([CP003790.1](#)), 02DC15 ([CP002806.1](#)), 01DC11 ([CP002805.1](#)), WC ([CP003796.1](#)), 01DC12 ([HF545614.1](#)), NJ1 ([CP003798.1](#)), CR009 ([LZRX01000000](#)), Ho Re upper ([LZRE01000000](#)) and PoAn ([LZRG01000000](#)). For *C. pec_HP* alignment, besides MC/Marsbar, we used the gene alleles from E58 ([CP002608.1](#)), P787 ([CP004035.1](#)), W73 ([CP004034.1](#)), IPA ([NZ_CM002311.1](#)), NSW/Bov/SBE ([NZ_JWHE00000000.1](#)), L71 ([LFRL01000000](#)), L17 ([LFRK01000001](#)), L1 ([LFRH00000000](#)), DBDeUG ([NZ_CM002308.1](#)), SA/K2/UGT ([SRR1693792](#)), Nar/S22/Rec ([SRR1693794](#)) and Mer/Ovi1/Jnt ([SRR1693791](#)).

Species-specific LAMP primers were designed using the target sequences with the open-source Primer Explorer v5 software (Eiken Chemical Co., Tokyo, Japan) and licensed LAMP Designer 1.15 software (Premier Biosoft, Palo Alto, CA, USA). For both *C. pecorum* and *C. psittaci*, Primer Explorer v5 yielded five sets of four LAMP primers including two outer (forward F3 and backward B3) primers and two inner (forward inner FIP and backward inner BIP) primers targeting different regions of the target gene, while LAMP Designer yielded single best set of six LAMP primers including two outer primers (forward F3 and backward B3), two inner primers (forward inner FIP and backward inner BIP) and two loop primers (forward loop LF and backwards loop LB). All primers (as single or paired) were tested *in silico*, including analysing primer sequences in blast for species specificity and OligoAnalyser 3.1 (available from <http://sg.idtdna.com/calc/analyzer>) for primer dimerization, hairpins and melting temperatures.

After *in silico* and in LAMP reaction testing, a set of four primers designed by PrimerExplorer v5 and targeting a 209 bp region of the *C. pec_HP* gene (spanning from position 22 to 230) was selected for *C. pecorum* LAMP assays performed in this study. Additional loop primers (LF/LB) were also designed to accelerate amplification time and increase sensitivity. For *C. psittaci*, a set of six primers designed with LAMP Designer and targeting a 263 bp region of the *C. ps_0607* gene (spanning from position 286 to 548) was selected for LAMP assays performed in this study. The specificity of primer sequences was assessed *in silico* using discontinuousBLAST analyses. Amplicons generated by conventional PCR using outer F3 and B3 primers for both *C. psittaci* and *C. pecorum* were gel excised, purified using Roche High Pure purification kit, and sent to Australian Genome Research Facility (AGRF) for Sanger sequencing for sequence identity confirmation.

LAMP assay optimisation

Both *C. psittaci* and *C. pecorum* LAMP assays were carried out in a 25 μ L reaction volume. The reaction mixture consisted of 15 μ L Isothermal Master Mix ISO001 (Optigene, Horsham, UK), 5 μ L six primers mix (at 0.2 μ M F3 and B3, 0.8 μ M FIP and BIP, and 0.4 μ M LF and LB) and 5 μ L template, following LAMP assay run at 65 °C in the Genie III real-time fluorometer (Optigene, Horsham, UK), as per manufacturer instructions. Following determination of the most optimal conditions (fastest amplification time, fluorescence and annealing temperature), *C. psittaci* LAMP assays were run at 65 °C for 30 min followed by annealing step of 98–80 °C at a rate of 0.05 °C/s, while *C. pecorum* LAMP assays were run using the same temperature and annealing conditions, however for 45 min. A negative control (LAMP mix only) was included in each run. Both *C. psittaci* and *C. pecorum* LAMP assays were performed on a thermal cycle heating block at 65 °C for 30 min, following detection of amplicons by electrophoresis on a 1.5% ethidium bromide agarose gel and visualisation under UV. In addition, several *C. pecorum* LAMP assays were conducted using the four primer set, two outer (F3 and B3) and two inner (FIP and BIP) primers, on a heating block at 65 °C for 45 min.

After the assay optimisation, LAMP testing was evaluated using previously tested clinical samples, previously characterised isolates and untested new samples. *C. pecorum*-presumptive samples were simultaneously tested using our in-house *C. pecorum*-specific qPCR assay (Marsh *et al.*, 2011), while *C. psittaci*-presumptive samples were tested using a pan-*Chlamydiales* qPCR assay with primers 16SIGF and 16SIGR targeting the 298 bp 16S rRNA fragment (Everett, Bush & Andersen, 1999). Amplicon sequencing was used for the latter assay to confirm species identity. The qPCR assays were carried out in a 20 μ L total volume, consisting of 10 μ L SYBRTM Green PCR Master Mix (Life Technologies Australia Pty Ltd., Scoresby, Victoria, Australia), 1 μ L of each 10 μ M forward and reverse primer, 3 μ L miliqH₂O, and 5 μ L DNA template. The qPCR assays were run for 35 cycles (Ct), and in each qPCR assay a positive (cultured *C. pecorum* and/or *C. psittaci* DNA) and negative (miliqH₂O) controls were included. Based on the qPCR standard curve and the number of running cycles, samples amplifying at >30 Ct (and/or equivalent detected genome copy number) were considered negative. The 23 *C. psittaci*-presumptive equine samples were also tested with a *C. psittaci*-specific qPCR assay targeting the 16S rRNA gene/16S-23S rRNA spacer gene (Madico *et al.*, 2000) at the State Veterinary Diagnostic Laboratory (SVDL), Elizabeth Macarthur Agricultural Institute (EMAI), Menangle, NSW, Australia. Samples amplifying at >39 Ct were considered negative. LAMP testing was performed in a blind fashion, by two different operators, unaware of qPCR results.

Statistical analyses

For each assay, we compared the performance of two tests evaluated in the same population by calculating Kappa and overall agreement, as well as estimated sensitivity and specificity (with specified Clopper–Pearson (exact) confidence limits) of LAMP compared to the known reference (gold standard) qPCR test using EpiTools online (Sergeant, 2017). It is suggested the Kappa value be interpreted as follows: values ≤ 0 as indicating no agreement

and 0.01–0.20 as none to slight, 0.21–0.40 as fair, 0.41–0.60 as moderate, 0.61–0.80 as substantial, and 0.81–1.00 as almost perfect agreement.

RESULTS AND DISCUSSION

With the emergence of new spill-over threats posed by *C. psittaci* (Laroucau *et al.*, 2015; Jelocnik *et al.*, 2017), there is an increasing need for rapid diagnostic tools for this pathogen, particularly for those that may have practical application in the field or clinical setting. There are specific needs for *C. pecorum* POC tests as well in both the veterinary care and treatment of infected domesticated and native animals, particularly in settings where veterinary diagnostic testing is logistically challenging. In the present study, to the best of our knowledge, we describe the first development of novel, rapid and robust *C. psittaci*-specific and *C. pecorum*-specific LAMP assays that are able to detect these bacteria in clinical samples in either the laboratory or POC settings.

C. psittaci and *C. pecorum* LAMP development

A *C. psittaci*-specific gene (*C.ps_0607*) was previously characterised as a conserved gene sequence present only in *C. psittaci* genomes, and absent from all other related chlamydial species (Voigt, Schöfl & Saluz, 2012). BLAST analyses and alignment of the *C.ps_0607* gene sequences, including those from recently described human, bird and equine Australian isolates, confirmed species specificity and sequence conservation. Between 0 and 13 single nucleotide polymorphisms (SNPs) were observed amongst strains (100–95.1% sequence identity) based on a 263 bp alignment of *C.ps_0607* gene sequences, including that from the most distant *C. psittaci* NJ1 taxon (Fig. S1A). Similarly, the *C. pecorum* HP gene (denoted *CpecG_0573* locus in Marsbar strain) was determined as a highly conserved species-specific sequence following BLAST analysis against publicly available sequences. Using an alignment of HP gene sequences from 14 publicly available *C. pecorum* genomes, there were only two SNPs in the 209 bp region to be targeted by LAMP (Fig. S1B).

Although multiple LAMP primer sets were predicted, LAMP primer sets denoted in Fig. 1 were chosen for further assay development. For *C. psittaci* assays, a set designed using LAMP Explorer was utilised while, for *C. pecorum*, we used a set designed with PrimerExplorer (Table 1). After initial testing, some of the predicted primer sets were discarded due to (i) potential cross-amplification associated with a lack of specificity of the target primer; (ii) not achieving an amplification signal in the fluorometer; and (iii) amplifying non-specific targets, including positive amplification in negative controls (data not shown). While we achieved initial amplification of a *C. psittaci* single copy dilution in a 30 min assay using the designed LAMP primer set, initial reaction times for a *C. pecorum* single copy amplification averaged 50 min. In order to accelerate amplification times for *C. pecorum*, we additionally designed a pair of Loop primers for the *C. pecorum* set which decreased the amplification of a single copy to 30 min.

Species-specificity for *C. psittaci* and *C. pecorum* LAMP targets was tested in the developed LAMP assays using DNA extracts from 12 *C. psittaci* and 18 *C. pecorum* cultured isolates, DNA extracts from other chlamydial species and a range of DNA extracts from other bacteria. Positive amplification as assessed by the presence of an observable

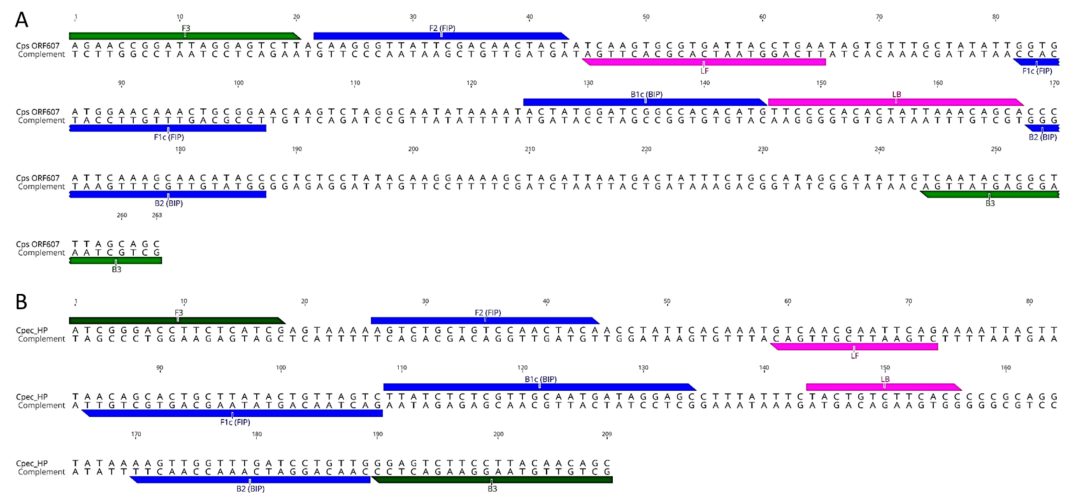


Figure 1 LAMP primer sequences and positions in the target gene regions. (A) *C. psittaci* LAMP primer set; and (B) *C. pecorum* LAMP primer set. Outer F3 and B3 primers are indicated in green, inner FIP and BIP in blue, and loop LF and BL in pink colour.

amplification curve characterised by a specific melt was observed only for the target species in their respective assays (Table S1). No amplification curves were observed for any of the non-targeted chlamydial species or other bacteria included in our specificity assays (Table S1). The *C. pecorum* and *C. psittaci* LAMP assays did not amplify either the related chlamydial species or other bacteria included in our specificity assays. In this study, in contrast, a previously described “*C. pecorum*-specific” qPCR assay (Marsh et al., 2011; Wan et al., 2011) showed positive amplification and melt for *C. psittaci* and *C. pneumoniae* DNA samples.

The choice to use the *C. ps_0607* gene as a LAMP target was straight forward since it had been suggested for such a purpose in previous studies (Voigt, Schöfl & Saluz, 2012; Opota et al., 2015), For *C. pecorum*, however, we utilised our ongoing comparative genomics to select *C. pecorum*-specific and conserved *C.pec_HP* gene described in this study for the first time. *In silico* analyses and assay development confirmed species-specificity of this gene and its suitability for use in diagnostic assays. Previously published *C. pecorum* diagnostic assays targeted highly polymorphic genes such as *ompA* (Higgins et al., 2012; Yang et al., 2014), which may require the use of probes due to sequence variation, prolonging the detection time and increasing diagnostic costs. Our routinely used in house *C. pecorum*-specific assay which targets a 204 bp 16S rRNA fragment (Marsh et al., 2011; Wan et al., 2011) was simpler to use, however we have shown that this assay may cross-react with other related chlamydial species due to a lack of sufficient sequence variation in the region of the 16S rRNA gene targeted (Bachmann, Polkinghorne & Timms, 2014). For koala diagnostics where *C. pecorum* is the most abundant and prevalent chlamydial organism (Polkinghorne, Hanger & Timms, 2013), this cross-reactivity may not be of a big concern. For the veterinary diagnosis of infections in livestock where co-infections with several chlamydial species are common (Lenzko et al., 2011; Reinhold, Sachse & Kaltenboeck, 2011), this assay may be less

Table 1 LAMP primers set used in this study.

Name	Sequence 5'–3'	Position	Length
<i>C. psittaci</i> LAMP primers			
F3	AGAACCGGATTAGGAGTCTT	286	20
B3	GCTGCTAAAGCGAGTATTGA	548	20
FIP(F1c + F2)	TCCGCAGTTTGTTCATCACCCAA GGGTTATTTCGACAACACTACT		43
BIP(B1c + B2)	ACTATGGATCGGCCACACATGGG TATGTTGCTTTGAATGGG		41
LoopF	TTCAGGTAATCACGCACTTGA	350	21
LoopB	TTCCCCACACTATTAACAGCA	431	22
F2	CAAGGGTTATTTCGACAACACTACT	307	22
F1c	TCCGCAGTTTGTTCATCACCC	387	21
B2	GGTATGTTGCTTTGAATGGG	472	20
B1c	ACTATGGATCGGCCACACATG	410	21
<i>C. pecorum</i> LAMP primers			
F3	ATCGGGACCTTCTCATCG	22	18
B3	GCTGTTGTAAGGAAGACTCC	230	20
FIP(F1c + F2)	GACTAACAGTATAAGCAGTGCTG TTAGTCTGCTGTCCAACACTACA		44
BIP(B1c + B2)	TTATCTCTCGTTGCAATGATAGGAG CCAACAGGATCAAACCAACTT		46
LoopF	CTGAATTCGTTGAC	93	14
LoopB	TACTGTCTTCACC	165	12
F2	AGTCTGCTGTCCAACACTACA	47	19
F1c	GACTAACAGTATAAGCAGTGCTGTT	129	25
B2	CAACAGGATCAAACCAACTT	210	20
B1c	TTATCTCTCGTTGCAATGATAGGAGC	130	26

suitable. Using the *C. pecorum*-specific HP gene as a target in different diagnostic assays would hence seem promising.

Performance of the *C. psittaci* and *C. pecorum* LAMP assays

The sensitivity of the LAMP assays was evaluated using 5 μ L cultured *C. psittaci* and *C. pecorum* gDNA in 10-fold serial dilutions as a template in assays performed in triplicate in separate runs. The limits of detection of the LAMP assays were conservatively 10 copies for *C. psittaci*, with 3/3 (100%) positive amplification for 10 copy dilutions for *C. psittaci*, and one copy for *C. pecorum*, with 3/3 (100%) positive amplifications for a single copy dilution of *C. pecorum* DNA (Tables 2 and 3). In the final and optimised LAMP assays, the mean amplification time detecting the lower limit (a single copy) for *C. psittaci* was 14.23 min with an average 84.45 °C melt (Table 2) while, for *C. pecorum*, it was 24 min with an average 83.42 °C melt (Table 3). Comparing the two newly developed assays, *C. psittaci* LAMP had the faster run time than that of *C. pecorum* LAMP. This difference in assays kinetics could be attributed to the improved *C. psittaci* LAMP primers design, as they were predicted by the LAMP Designer software (Nagamine, Hase & Notomi, 2002). As

Table 2 *C. psittaci* LAMP assay^a sensitivity.

Dilution ^d	Time to amplify (min)	Melt (°C)	Time (Mean + SD)	Melt (Mean + SD)
10 ⁶	5.15	84.43		
10 ⁶	5.00	84.46	5.10, 0.09	84.49, 0.08
10 ⁶	5.15	84.58		
10 ⁵	6.30	84.34		
10 ⁵	6.45	84.33	6.30, 0.15	84.37, 0.06
10 ⁵	6.15	84.43		
10 ⁴	7.15	84.59		
10 ⁴	7.30	84.58	7.25, 0.09	84.56, 0.04
10 ⁴	7.30	84.51		
10 ³	8.45	84.46		
10 ³	8.15	84.43	8.25, 0.173	84.44, 0.01
10 ³	8.15	84.44		
100	9.15	84.48		
100	9.30	84.39	9.30, 0.15	84.46, 0.06
100	9.45	84.51		
10	12.00	84.41		
10	11.00	84.35	11.33, 0.58	84.38, 0.03
10	11.00	84.39		
1	16.00	84.44		
1	0.00	0	14.23, 2.51	84.34, 0.14
1	12.45	84.24		
0.1	25.25	84.20		
0.1	– ^b	–	–	84.20
0.1	–	84.20 ^c		

Notes.

^aThe assay was performed in Genie III Real-time fluorometer, with the amplification times and annealing temperatures recorded at the end of each run. The samples were tested in three different runs.

^bNo amplification detected.

^cNo amplification, but melt and annealing curve recorded.

^dTemplate was serially diluted *C. psittaci* CR009 gDNA which genome copy number was determined by qPCR.

we additionally designed Loop primers for *C. pecorum*, we can anticipate an improvement in the *C. pecorum* assay kinetics by re-designing the loop primers (e.g., extending the sequence to 20–22 bp), as well as testing LAMP mixes in different ratios and with improved polymerases.

In order to test the reproducibility of our LAMP assays, we tested a subset of *C. pecorum* and *C. psittaci* PCR positive samples (Table 4). All samples were run in a “blind fashion”, in triplicate and in separate runs by two different operators. For both assays, the amplification times and melts of each sample between the runs were very similar, with 0 to 1.5 min (SDs ranging from 0–0.98) difference in amplification times for each sample, and 0.03 to 0.83 °C (SDs ranging from 0.02–0.26) difference in melt for each sample. Congruence between the runs performed by different operators indicates that both LAMP assays described in this study are highly reproducible, and can detect the target organism in less than 30 min even when in low infectious loads of <10 copies.

Table 3 *C. pecorum* LAMP assay^c sensitivity.

Dilution ^f	Time to amplify (min)	Melt (°C)	Time (Mean + SD)	Melt (Mean + SD)
10 ⁷ k ^a	10.00	83.23		
10 ⁷ k	10.45	83.37	10.23, 0.32	83.30, 0.1
10 ⁶ k	13.15	83.57		
10 ⁶ s ^b	13.15	83.33	12.92, 0.40	83.51, 0.16
10 ⁶ c ^c	12.45	83.62		
10 ⁵ k	14.00	83.52		
10 ⁵ s	14.00	83.35	14.10, 0.17	83.48, 0.11
10 ⁵ c	14.30	83.57		
10 ⁴ k	15.45	83.56		
10 ⁴ s	16.45	83.33	16.30, 0.78	83.44, 0.11
10 ⁴ c	17.00	83.42		
10 ³ k	19.00	83.50		
10 ³ s	17.45	83.39	18.87, 1.35	83.45, 0.06
10 ³ c	20.15	83.47		
100k	20.15	83.47		
100s	18.45	83.09	20.35, 2.00	83.33, 0.21
100c	22.45	83.42		
10k	22.30	83.52		
10s	21.00	83.42	22.43, 1.50	83.42, 0.1
10c	24.00	83.33		
1k	23.15	83.52		
1s	22.30	83.42	23.92, 2.11	83.41, 0.12
1c	26.30	83.28		
0.1k	36.00	83.41		
0.1s	— ^d	83.43	34.65, 1.91	83.39, 0.06
0.1c	33.30	83.33		

Notes.^aKoala Marsbar isolate.^bSheep IPA isolate.^cCattle E58 isolate.^dNo amplification, but melt and annealing curve recorded.^eThe assay was performed in Genie III Real-time fluorometer, with the amplification times and annealing temperatures recorded at the end of each run. The samples were tested in different runs.^fTemplate was serially diluted *C. pecorum* gDNA which genome copy number was determined by qPCR.**Pathogen detection in clinical samples using newly developed LAMP**

For *C. psittaci*, a total of 26 DNA extracts from clinical samples were tested with both *C. psittaci* LAMP and qPCR assays (Table S2). For these analyses, samples with >20 min amplification time were considered negative for LAMP, while for qPCR, samples with <20 genome copy/reaction and/or >30 Ct (quantification cycle) were considered negative, based on the qPCR standard curve and the number of running cycles used for this testing. As observed in Table S2 and based on above cut-off values, 24/26 (92.3%) samples were congruent between the two tests, with 11 samples positive and 13 samples negative by both (Table 5). For 2/26 (7.7%) where there was disagreement, one sample was LAMP positive but qPCR negative, and another was qPCR positive but *C. psittaci* LAMP negative. Based

Table 4 Reproducibility of the LAMP testing using clinical and cultured samples.

Samples	Run ^a	Time to amplify (min)	Melt (°C)	Time (Mean + SD)	Melt (Mean + SD)
<i>C. pecorum</i> positive samples					
Koala rectal swab	1	20.15	83.44	20.53, 0.54	83.32, 0.16
	2	20.30	83.37		
	3	21.15	83.14		
Marsbar DNA	1	13.50	83.50	13.27, 0.20	83.55, 0.06
	2	13.15	83.52		
	3	13.15	83.62		
Koala A2 DNA	1	12.00	83.35	11.43, 0.51	83.41, 0.05
	2	11.00	83.45		
	3	11.30	83.43		
RI koala UGT swab	1	17.00	83.34	17.72, 0.62	83.21, 0.12
	2	18.00	83.21		
	3	18.15	83.09		
L14 DNA	1	13.15	83.53	13.15, 0	83.50, 0.02
	2	13.15	83.50		
	3	13.15	83.48		
HsLuRz DNA	1	13.45	83.49	13.63, 0.32	83.40, 0.08
	2	13.45	83.36		
	3	14.00	83.34		
K20 cloaca swab	1	22.00	82.83	22.2, 0.23	83.01, 0.19
	2	22.15	83.00		
	3	22.45	83.20		
<i>C. psittaci</i> positive samples					
Cr009 DNA	1	6.45	84.30	6.40, 0.09	84.33, 0.03
	2	6.45	84.36		
	3	6.30	84.34		
HoRE DNA	1	5.00	84.46	5.10, 0.08	84.45, 0.14
	2	5.15	84.58		
	3	5.15	84.30		
B2 DNA	1	10.30	84.08	10.10, 0.17	84.17, 0.08
	2	10.00	84.20		
	3	10.00	84.24		
Horse placental swab	1	11.15	82.90	10.58, 0.49	83.19, 0.26
	2	10.30	83.42		
	3	10.30	83.24		
Horse_pl DNA	1	10.30	84.53	10.87, 0.98	84.41, 0.18
	2	12.00	84.21		
	3	10.30	84.50		

Notes.

^aThe assay was performed in Genie III Real-time fluorometer, with the amplification times and annealing temperatures recorded at the end of each run. The samples were tested in three different runs by two different operators.

Table 5 Comparison of the *C. psittaci* LAMP and qPCR methods for the organism detection in clinical samples.

Test	qPCR +ve	qPCR –ve	qPCR Total
LAMP +ve	11	1	12
LAMP –ve	1	13	14
LAMP Total	12	14	26

Table 6 Comparison of the *C. pecorum* LAMP and qPCR methods for the organism detection in clinical samples.

Test	16s +ve	16s –ve	16s Total
LAMP +ve	29	7	36
LAMP –ve	3	24	27
LAMP Total	32	31	63

on these results, the Kappa value was calculated at 0.85 (95% CI [0.64–1.05]) indicating an almost perfect agreement between the tests. The overall sensitivity of the *C. psittaci* LAMP was 91.7% (Clopper–Pearson 95% CI [0.62–0.99]) and with 92.9% (Clopper–Pearson 95% CI [0.66–0.99]) specificity, compared to the qPCR used in this study. In addition, a subset of 23 samples was also tested independently by a third party. Using a cut off of >Ct 39 as negative, 19/23 (82.60 %) of these test results were in congruence with our *C. psittaci* LAMP results (Table S2).

For *C. pecorum*, we tested a total of 63 DNA extracts from clinical samples from several animal hosts by both LAMP and qPCR (Table S3). For these analyses, samples with >30 min amplification time were considered negative for LAMP, while for qPCR, samples with <35 genome copy /reaction and/or >30 Ct were considered negative based on the standard curve and number of run cycles used for this testing. For the 63 clinical samples, the overall congruence was 84.1% with a Kappa value of 0.68 (95% CI [0.50–0.86]), indicating substantial agreement between the tests. Congruent results between tests were obtained for 53 samples, while there were 10 discrepant samples using the above cut off for *C. pecorum* (Table 6). The overall sensitivity of *C. pecorum* LAMP was 90.6 % (Clopper–Pearson 95% CI [0.75–0.98]), while specificity was 77.4 % (Clopper–Pearson 95% CI [0.59–0.90]) in comparison to the qPCR assay. A subset of 36 *C. pecorum* samples was also tested in a thermal cycler using the newly developed LAMP and results were determined as an end point detection. For this experiment, 34/36 (94.4%) samples were congruent between LAMP performed in fluorometer and in a thermal cycler (Table S3), demonstrating the robustness of the *C. pecorum* LAMP (Fig. S2).

Considering that the qPCR assay used in this study to quantify and detect *C. psittaci* is chlamydial genus rather species specific (Everett, Bush & Andersen, 1999), high congruence observed for *C. psittaci* assays could be attributed to testing a limited set of samples taken from hosts with presumptive *C. psittaci* chlamydiosis. Lower congruence between the *C. pecorum*-specific assays could be due to technical and experimental aspects and characteristics (such as the assay efficiency, analytical sensitivity, template preparation)

Table 7 Comparison of *C. pecorum* LAMP and qPCR for organism detection using rapidly processed swab samples and their DNA extracts.

Sample	LAMP ^a result for swab suspension	qPCR ^b result for swab suspension	LAMP result for DNA extract	qPCR result for DNA extract	LAMP result for “spiked” swab suspension	LAMP result for “spiked” DNA extract	qPCR result for “spiked” swab suspension	qPCR result for “spiked” DNA extract
K1 ocular ^c	NEG	NEG	0.00/83.49	NEG	NEG	–	NEG	–
K6 ocular ^c	NEG	NEG	21.00/83.23	3 × 10 ³ (Ct 20)	NEG	–	NEG	–
K9 ocular ^c	NEG	NEG	25.45/83.39	287 (Ct 24)	NEG	–	NEG	–
K2 ocular ^c	NEG	NEG	NEG	NEG	NEG	–	NEG	–
R1 eye	25.45/83.39	222 (Ct 25)	20.15/83.27	750 (Ct 24)	–	–	–	–
R1 cloaca	30.00/83.34	NEG	NEG	NEG	11.15/83.47	12.15/83.42	5 × 10 ³ (Ct 17)	1.5 × 10 ³ (Ct 18)
K eye	27.00/83.15	NEG	0.00/83.35	NEG	–	–	–	–
Koala 2 eye	NEG	NEG	NEG	NEG	11.00/83.51	11.00/83.40	1.2 × 10 ³ (Ct 19)	1.1 × 10 ⁴ (Ct 15)
Koala 2 cloaca	27.30/83.77	116 (Ct 26)	21.30/83.49	375 (Ct 25)	–	–	–	–
Will Cloaca	0.00/83.77	NEG	NEG	NEG	12.00/83.45	11.00/83.34	1.5 × 10 ³ (Ct 19)	8 × 10 ³ (Ct 17)
23117 Eye	21.30/83.20	NEG	23.15/83.23	150 (Ct 25)	–	–	–	–
23117 Cloaca	22.00/83.29	NEG	24.00/83.15	90 (Ct 27)	–	–	–	–
Flyn eye	NEG	NEG	NEG	NEG	12.30/83.50	11.00/83.35	1.9 × 10 ³ (Ct 18)	8.3 × 10 ³ (Ct 16)
Tyke eye	NEG	NEG	NEG	NEG	12.00/83.44	10.45/83.40	1.3 × 10 ³ (Ct 19)	9 × 10 ³ (Ct 16)
Bill eye	NEG	NEG	NEG	NEG	12.15/83.49	10.45/83.34	1.2 × 10 ³ (Ct 19)	1 × 10 ⁴ (Ct 15)
Ray eye	NEG	NEG	NEG	NEG	12.45/83.49	11.00/83.40	4.7 × 10 ³ (Ct 17)	1 × 10 ⁴ (Ct 15)
Ray cloaca	NEG	NEG	NEG	NEG	12.15/83.43	11.00/83.30	700 (Ct 20)	9 × 10 ³ (Ct 16)
Koala F Eye	NEG	NEG	NEG	NEG	11.45/83.45	11.00/83.35	1.3 × 10 ³ (Ct 19)	1.1 × 10 ⁴ (Ct 15)

Notes.^aLAMP results are expressed as time to amplify (min) and melt (°C).^bqPCR results are expressed as copies/reaction and Ct value.^cRNA Later swabs.

(Bustin *et al.*, 2010) of the *C. pecorum* 16S qPCR assay used in this study. As a sidenote, we also evaluated the use of *C. psittaci* and *C. pecorum* LAMP targets (263 bp of the *C. ps_0607* and 209 bp *C. pec_HP* genes, respectively) using outer F3 and B3 primers in a fluorescence-based (SybrGreen) qPCR assays, if needed to estimate infectious loads of the pathogen. In this preliminary analyses, both targets seem suitable for use in qPCR assays as well, as we were able to detect low infectious load up to 10 copies/reaction in a sample.

Rapid swab processing

Rapid swab processing and using the swab suspension directly in LAMP assays were previously successfully evaluated for testing for respiratory syncytial virus from nasopharyngeal swabs (Mahony *et al.*, 2013) and rapid detection of *Streptococcus agalactiae* in vaginal swabs (McKenna *et al.*, 2017). A recent study also demonstrated that *C. trachomatis* can be detected directly from urine samples using the LAMP method (Jevtusevska *et al.*, 2016). In this study, we also evaluated rapid swab processing without DNA extraction in order to begin to assess the POC potential of these assays. A total of 18 swabs taken from conjunctival and urogenital sites from koalas with presumptive chlamydiosis, of which four were stored in RNA Later and 14 were dry, were used for this experiment (Table 7). Vigorously vortexed and heated swab suspension samples were directly used as a template in both *C. pecorum* LAMP reaction performed in fluorometer and qPCR assay. We also performed DNA extraction from the swabs to be used as a comparison to rapid swab processing. We did not detect *C. pecorum* DNA in any of the RNA Later suspensions either by LAMP nor qPCR assay (Table 7), in contrast to detecting *C. pecorum* in 50% (2/4) of the DNA extracts from the swabs by both methods. Using the rapidly processed swab suspension as a template, *C. pecorum* was detected in 6/14 by LAMP, and only 2/14 by qPCR (Table 7). The swab suspension LAMP results were 92.8% (13/14) congruent to the LAMP results and 85.7% congruent (12/14) to the qPCR results using the swab's paired DNA sample. In order to evaluate the potential presence of inhibitors in our samples, we "spiked" negative swab suspensions and its paired DNA samples with known amounts of *C. pecorum* (1×10^4 copies/reaction). As observed in Table 7, we detected *C. pecorum* by both LAMP and qPCR in "spiked" negative samples derived from dry swabs. No *C. pecorum* was detected in "spiked" RNA Later swab suspension, indicating the potential presence of inhibitors in these reactions. Our results suggest that the LAMP assays are capable of amplifying specific amplification products from crude DNA extracts.

Further work is additionally required to enhance the POC capabilities of these new chlamydial LAMP assays to meet the clinical need including (i) the evaluation of rapid swab processing methods using commercially available DNA release portable devices and/or sample preparation using microfluidic support; (ii) alternative amplification detection methods such as visible colorimetric or turbidimetric change and/or solid-phase 'dipstick' tests (Maffert *et al.*, 2017). With further development and the aforementioned focus on the preparation of these assays at the POC (Parida *et al.*, 2008; Tomita *et al.*, 2008), it is anticipated that both LAMP tests described in this study may fill an important niche in the repertoire of ancillary diagnostic tools available to clinicians.

ACKNOWLEDGEMENTS

We thank Prof. James Mahony, Dr. Catherine Chicken, Dr. Joan Carrick, Dr. Ian Marsh, Narelle Sales and Dr. Bill Lott for their helpful advice on POC assays. We also thank Dr. Brendon O'Rourke, Sankhya Bommana, Sharon Nyari, Noa Ziklo and Alyce Taylor-Brown for provision of DNA samples used in this study. We also thank Sean McDonald, Geneworks, Australia, for providing us with the Genie III Fluorometer.

ADDITIONAL INFORMATION AND DECLARATIONS

Funding

This work was funded by the University of the Sunshine Coast Research Seed Grant awarded to Martina Jelocnik. The funders had no role in study design, data collection and analysis, decision to publish, or preparation of the manuscript.

Grant Disclosures

The following grant information was disclosed by the authors:
University of the Sunshine Coast Research Seed.

Competing Interests

The authors declare there are no competing interests.

Author Contributions

- Martina Jelocnik conceived and designed the experiments, performed the experiments, analyzed the data, contributed reagents/materials/analysis tools, wrote the paper, prepared figures and/or tables, reviewed drafts of the paper.
- Md. Mominul Islam, Danielle Madden, Cheryl Jenkins and Scott Carver performed the experiments, analyzed the data, reviewed drafts of the paper.
- James Branley performed the experiments, reviewed drafts of the paper.
- Adam Polkinghorne analyzed the data, contributed reagents/materials/analysis tools, reviewed drafts of the paper.

Animal Ethics

The following information was supplied relating to ethical approvals (i.e., approving body and any reference numbers):

The use of these swabs was considered by the University of The Sunshine Coast (USC) Animal Ethics Committee and the need for further ethics consideration was waived under exemption AN/E/17/19.

Data Availability

The following information was supplied regarding data availability:

The raw data has been supplied as [Supplementary Files](#).

Supplemental Information

Supplemental information for this article can be found online at <http://dx.doi.org/10.7717/peerj.3799#supplemental-information>.

REFERENCES

- Bachmann NL, Polkinghorne A, Timms P. 2014. Chlamydia genomics: providing novel insights into chlamydial biology. *Trends in Microbiology* 22:464–472 DOI 10.1016/j.tim.2014.04.013.
- Branley J, Bachmann NL, Jelocnik M, Myers GS, Polkinghorne A. 2016. Australian human and parrot *Chlamydia psittaci* strains cluster within the highly virulent 6BC clade of this important zoonotic pathogen. *Scientific Reports* 6:30019 DOI 10.1038/srep30019.
- Branley JM, Roy B, Dwyer DE, Sorrell TC. 2008. Real-time PCR detection and quantitation of *Chlamydophila psittaci* in human and avian specimens from a veterinary clinic cluster. *European Journal of Clinical Microbiology and Infectious Diseases* 27:269–273 DOI 10.1007/s10096-007-0431-0.
- Branley JM, Weston KM, England J, Dwyer DE, Sorrell TC. 2014. Clinical features of endemic community-acquired psittacosis. *New Microbes New Infections* 2:7–12 DOI 10.1002/2052-2975.29.
- Burnard D, Polkinghorne A. 2016. Chlamydial infections in wildlife—conservation threats and/or reservoirs of ‘spill-over’ infections? *Veterinary Microbiology* 196:78–84 DOI 10.1016/j.vetmic.2016.10.018.
- Bustin SA, Beaulieu JF, Huggett J, Jaggi R, Kibenge FS, Olsvik PA, Penning LC, Toegel S. 2010. MIQE precis: practical implementation of minimum standard guidelines for fluorescence-based quantitative real-time PCR experiments. *BMC Molecular Biology* 11:74 DOI 10.1186/1471-2199-11-74.
- Chan J, Doyle B, Branley J, Sheppard V, Gabor M, Viney K, Quinn H, Janover O, McCready M, Heller J. 2017. An outbreak of psittacosis at a veterinary school demonstrating a novel source of infection. *One Health* 3:29–33 DOI 10.1016/j.onehlt.2017.02.003.
- Choopara I, Arunrut N, Kiatpathomchai W, Dean D, Somboonna N. 2017. Rapid and visual *Chlamydia trachomatis* detection using loop-mediated isothermal amplification and hydroxynaphthol blue. *Letters in Applied Microbiology* 64:51–56 DOI 10.1111/lam.12675.
- Everett KDE, Bush RM, Andersen AA. 1999. Emended description of the order *Chlamydiales*, proposal of *Parachlamydiaceae* fam. nov. and *Simkaniaceae* fam. nov., each containing one monotypic genus, revised taxonomy of the family *Chlamydiaceae*, including a new genus and five new species, and standards for the identification of organisms. *International Journal of Systematic Bacteriology* 49:415–440 DOI 10.1099/00207713-49-2-415.
- Gaede W, Reckling KF, Dresenkamp B, Kenklies S, Schubert E, Noack U, Irmischer HM, Ludwig C, Hotzel H, Sachse K. 2008. *Chlamydophila psittaci* infections in humans during an outbreak of psittacosis from poultry in Germany. *Zoonoses and Public Health* 55:184–188 DOI 10.1111/j.1863-2378.2008.01108.x.

- Geens T, Dewitte A, Boon N, Vanrompay D. 2005.** Development of a *Chlamydophila psittaci* species-specific and genotype-specific real-time PCR. *Veterinary Research* **36**:787–797 DOI [10.1051/vetres:2005035](https://doi.org/10.1051/vetres:2005035).
- Gonzalez-Astudillo V, Allavena R, McKinnon A, Larkin R, Henning J. 2017.** Decline causes of koalas in South East Queensland, Australia: a 17-year retrospective study of mortality and morbidity. *Scientific Reports* **7**:42587 DOI [10.1038/srep42587](https://doi.org/10.1038/srep42587).
- Hanger J, Loader J, Wan C, Beagley KW, Timms P, Polkinghorne A. 2013.** Comparison of antigen detection and quantitative PCR in the detection of chlamydial infection in koalas (*Phascolarctos cinereus*). *The Veterinary Journal* **195**:391–393 DOI [10.1016/j.tvjl.2012.07.024](https://doi.org/10.1016/j.tvjl.2012.07.024).
- Higgins DP, Beninati T, Meek M, Irish J, Griffith JE. 2012.** Within-population diversity of koala *Chlamydophila pecorum* at *ompA* VD1-VD3 and the ORF663 hypothetical gene. *Veterinary Microbiology* **156**:353–358 DOI [10.1016/j.vetmic.2011.11.005](https://doi.org/10.1016/j.vetmic.2011.11.005).
- Jelocnik M, Bachmann NL, Kaltenboeck B, Waugh C, Woolford L, Speight KN, Gillett A, Higgins DP, Flanagan C, Myers GS, Timms P, Polkinghorne A. 2015a.** Genetic diversity in the plasticity zone and the presence of the chlamydial plasmid differentiates *Chlamydia pecorum* strains from pigs, sheep, cattle, and koalas. *BMC Genomics* **16**:893 DOI [10.1186/s12864-015-2053-8](https://doi.org/10.1186/s12864-015-2053-8).
- Jelocnik M, Branley J, Heller J, Raidal S, Alderson S, Galea F, Gabor M, Polkinghorne A. 2017.** Multilocus sequence typing identifies an avian-like *Chlamydia psittaci* strain involved in equine placentitis and associated with subsequent human psittacosis. *Emerging Microbes and Infection* **6**:e7 DOI [10.1038/emi.2016.135](https://doi.org/10.1038/emi.2016.135).
- Jelocnik M, Self R, Timms P, Borel N, Polkinghorne A. 2015b.** Novel sequence types of *Chlamydia pecorum* infect free-ranging Alpine ibex (*Capra ibex*) and red deer (*Cervus elaphus*) in Switzerland. *Journal of Wildlife Diseases* **51**:479–483 DOI [10.7589/2014-08-220](https://doi.org/10.7589/2014-08-220).
- Jevtusevskaia J, Uusna J, Andresen L, Krolov K, Laanpere M, Grellier T, Tulp I, Langel U. 2016.** Combination with antimicrobial peptide lyses improves loop-mediated isothermal amplification based method for *Chlamydia trachomatis* detection directly in urine sample. *BMC Infectious Diseases* **16**:329 DOI [10.1186/s12879-016-1674-0](https://doi.org/10.1186/s12879-016-1674-0).
- Kawai Y, Miyashita N, Kishi F, Tabuchi M, Oda K, Yamaguchi T, Kawasaki K, Yamazaki T, Ouchi K. 2009.** Development and evaluation of a loop-mediated isothermal amplification method for the rapid detection of *Chlamydophila pneumoniae*. *European Journal of Clinical Microbiology and Infectious Diseases* **28**:801–805 DOI [10.1007/s10096-009-0710-z](https://doi.org/10.1007/s10096-009-0710-z).
- Kearse M, Moir R, Wilson A, Stones-Havas S, Cheung M, Sturrock S, Buxton S, Cooper A, Markowitz S, Duran C, Thierer T, Ashton B, Meintjes P, Drummond A. 2012.** Geneious Basic: an integrated and extendable desktop software platform for the organization and analysis of sequence data. *Bioinformatics* **28**:1647–1649 DOI [10.1093/bioinformatics/bts199](https://doi.org/10.1093/bioinformatics/bts199).
- Knittler MR, Sachse K. 2015.** *Chlamydia psittaci*: update on an underestimated zoonotic agent. *Pathogens and Disease* **73**:1–15 DOI [10.1093/femspd/ftu007](https://doi.org/10.1093/femspd/ftu007).

- Laroucau K, Aaziz R, Meurice L, Servas V, Chossat I, Royer H, de Barbeyrac B, Vaillant V, Moyen JL, Meziani F, Sachse K, Rolland P. 2015. Outbreak of psittacosis in a group of women exposed to *Chlamydia psittaci*-infected chickens. *Euro Surveill* 20(24):21155.
- Lenzko H, Moog U, Henning K, Lederbach R, Diller R, Menge C, Sachse K, Sprague L. 2011. High frequency of chlamydial co-infections in clinically healthy sheep flocks. *BMC Veterinary Research* 7:29 DOI 10.1186/1746-6148-7-29.
- Madico G, Quinn TC, Boman J, Gaydos CA. 2000. Touchdown enzyme time release-PCR for detection and identification of *Chlamydia trachomatis*, *C. pneumoniae*, and *C. psittaci* using the 16S and 16S-23S spacer rRNA genes. *Journal of Clinical Microbiology* 38:1085–1093.
- Maffert P, Reverchon S, Nasser W, Rozand C, Abaibou H. 2017. New nucleic acid testing devices to diagnose infectious diseases in resource-limited settings. *European Journal of Clinical Microbiology and Infectious Diseases* Epub ahead of print DOI 10.1007/s10096-017-3013-9.
- Mahony J, Chong S, Bulir D, Ruyter A, Mwawasi K, Waltho D. 2013. Development of a sensitive loop-mediated isothermal amplification assay that provides specimen-to-result diagnosis of respiratory syncytial virus infection in 30 minutes. *Journal of Clinical Microbiology* 51:2696–2701 DOI 10.1128/jcm.00662-13.
- Mansour SM, Ali H, Chase CC, Cepica A. 2015. Loop-mediated isothermal amplification for diagnosis of 18 World Organization for Animal Health (OIE) notifiable viral diseases of ruminants, swine and poultry. *Animal Health Research Reviews* 16:89–106 DOI 10.1017/s1466252315000018.
- Marsh J, Kollipara A, Timms P, Polkinghorne A. 2011. Novel molecular markers of *Chlamydia pecorum* genetic diversity in the koala (*Phascolarctos cinereus*). *BMC Microbiology* 11:77 DOI 10.1186/1471-2180-11-77.
- McKenna JP, Cox C, Fairley DJ, Burke R, Shields MD, Watt A, Coyle PV. 2017. Loop-mediated isothermal amplification assay for rapid detection of *Streptococcus agalactiae* (group B streptococcus) in vaginal swabs—a proof of concept study. *Journal of Medical Microbiology* 66:294–300 DOI 10.1099/jmm.0.000437.
- Menard A, Clerc M, Subtil A, Megraud F, Bebear C, de Barbeyrac B. 2006. Development of a real-time PCR for the detection of *Chlamydia psittaci*. *Journal of Medical Microbiology* 55:471–473 DOI 10.1099/jmm.0.46335-0.
- Nagamine K, Hase T, Notomi T. 2002. Accelerated reaction by loop-mediated isothermal amplification using loop primers. *Molecular and Cellular Probes* 16:223–229 DOI 10.1006/mcpr.2002.0415.
- Notomi T, Mori Y, Tomita N, Kanda H. 2015. Loop-mediated isothermal amplification (LAMP): principle, features, and future prospects. *Journal of Microbiology* 53:1–5 DOI 10.1007/s12275-015-4656-9.
- Opota O, Jatou K, Branley J, Vanrompay D, Erard V, Borel N, Longbottom D, Greub G. 2015. Improving the molecular diagnosis of *Chlamydia psittaci* and *Chlamydia abortus* infection with a species-specific duplex real-time PCR. *Journal of Medical Microbiology* 64:1174–1185 DOI 10.1099/jmm.0.000139.

- Parida M, Sannarangaiah S, Dash PK, Rao PV, Morita K. 2008.** Loop mediated isothermal amplification (LAMP): a new generation of innovative gene amplification technique; perspectives in clinical diagnosis of infectious diseases. *Reviews in Medical Virology* **18**:407–421 DOI [10.1002/rmv.593](https://doi.org/10.1002/rmv.593).
- Polkinghorne A, Hanger J, Timms P. 2013.** Recent advances in understanding the biology, epidemiology and control of chlamydial infections in koalas. *Veterinary Microbiology* **165**:214–223 DOI [10.1016/j.vetmic.2013.02.026](https://doi.org/10.1016/j.vetmic.2013.02.026).
- Reinhold P, Sachse K, Kaltenboeck B. 2011.** *Chlamydiaceae* in cattle: commensals, trigger organisms, or pathogens? *The Veterinary Journal* **189**:257–267 DOI [10.1016/j.tvjl.2010.09.003](https://doi.org/10.1016/j.tvjl.2010.09.003).
- Sachse K, Vretou E, Livingstone M, Borel N, Pospischil A, Longbottom D. 2009.** Recent developments in the laboratory diagnosis of chlamydial infections. *Veterinary Microbiology* **135**:2–21 DOI [10.1016/j.vetmic.2008.09.040](https://doi.org/10.1016/j.vetmic.2008.09.040).
- Sergeant ESG. 2017.** Epitools epidemiological calculators. Available at <http://epitools.ausvet.com.au>.
- Szymanska-Czerwinska M, Niemczuk K. 2016.** Avian Chlamydiosis zoonotic disease. *Vector Borne and Zoonotic Diseases* **16**:1–3 DOI [10.1089/vbz.2015.1839](https://doi.org/10.1089/vbz.2015.1839).
- Taylor-Brown A, Polkinghorne A. 2017.** New and emerging chlamydial infections of creatures great and small. *New Microbes New Infections* **18**:28–33 DOI [10.1016/j.nmni.2017.04.004](https://doi.org/10.1016/j.nmni.2017.04.004).
- Tomita N, Mori Y, Kanda H, Notomi T. 2008.** Loop-mediated isothermal amplification (LAMP) of gene sequences and simple visual detection of products. *Nature Protocols* **3**:877–882 DOI [10.1038/nprot.2008.57](https://doi.org/10.1038/nprot.2008.57).
- Voigt A, Schöfl G, Saluz HP. 2012.** The *Chlamydia psittaci* genome: a comparative analysis of intracellular pathogens. *PLOS ONE* **7**:e35097 DOI [10.1371/journal.pone.0035097](https://doi.org/10.1371/journal.pone.0035097).
- Walker E, Lee EJ, Timms P, Polkinghorne A. 2015.** *Chlamydia pecorum* infections in sheep and cattle: A common and under-recognised infectious disease with significant impact on animal health. *Veterinary Journal* **206**:252–260 DOI [10.1016/j.tvjl.2015.09.022](https://doi.org/10.1016/j.tvjl.2015.09.022).
- Walker E, Moore C, Shearer P, Jelocnik M, Bommana S, Timms P, Polkinghorne A. 2016.** Clinical, diagnostic and pathologic features of presumptive cases of *Chlamydia pecorum*-associated arthritis in Australian sheep flocks. *BMC Veterinary Research* **12**:193 DOI [10.1186/s12917-016-0832-3](https://doi.org/10.1186/s12917-016-0832-3).
- Wan C, Loader J, Hanger J, Beagley KW, Timms P, Polkinghorne A. 2011.** Using quantitative polymerase chain reaction to correlate *Chlamydia pecorum* infectious load with ocular, urinary and reproductive tract disease in the koala (*Phascolarctos cinereus*). *Australian Veterinary Journal* **89**:409–412 DOI [10.1111/j.1751-0813.2011.00827.x](https://doi.org/10.1111/j.1751-0813.2011.00827.x).
- Yang R, Jacobson C, Gardner G, Carmichael I, Campbell AJ, Ryan U. 2014.** Longitudinal prevalence and faecal shedding of *Chlamydia pecorum* in sheep. *Veterinary Journal* **201**:322–326 DOI [10.1016/j.tvjl.2014.05.037](https://doi.org/10.1016/j.tvjl.2014.05.037).